

Session location: Penn Station  
 Session site: n/a  
 Organizational affiliation: enviro club  
 Session environment: outdoors  
 Session type: Ambient  
 Session environment: n/a  
 Session Description: On the corner of RR Ave and Ferry St in Park  
 ACCESSLogger Serial Number: 99002  
 Logging began on: 03/06/2000 at 16:24:04  
 Logging stopped on: 03/06/2000 at 17:46:04  
 Data uploaded on: 03/06/2000 at 20:31:18  
 Pump has not been activated during session.  
 Samples were averaged and saved every (minutes): 1  
 Total samples in this upload: 82  
 Memory remaining: 6 days 20 hrs 34 minutes

SENSOR	UNITS	LO LIM	HI LIM
Barometric Pressure	in.-Hg	*	*
Carbon Monoxide	ppm	*	9
Nitrogen Dioxide	ppb	*	80
Ozone	ppb	*	120
Relative Humidity	%	30	60
Sulfur Dioxide	ppb	*	140
Temperature	Deg. F	*	*
Wind Direction	Deg.	*	*
Wind Speed	mph	*	*
Supply Voltage	V	*	*

\* indicates no limit was set

Data collected by: Randolph Kelly  
 City: Newark  
 State: NJ  
 Country: USA  
 Longitude: 50 Deg. 50 Min. W  
 Latitude: 50 Deg. 50 Min. N  
 Elev.(m): 50 m.

#### Air Quality Parameters

When evaluating outdoor air, the ACCESS EMS measures the same parameters as those measured by the EPA under the National Ambient Air Quality Standard promulgated by the Clean Air Act. In addition, other parameters, such as ultraviolet radiation, wind speed and wind direction, may be monitored.

The indoor environment has become an issue of concern over the past several years with the advent of new construction techniques and building materials which severely restrict the exchange of indoor and outdoor air. This \*could have a deleterious effect on the quality of indoor air,\* and, therefore, the quality of life. \*Many substances \*effect the quality of the indoor environment. The ACCESS EMS, depending upon configuration, can quantify a number of key indicators of both indoor and outdoor air quality including:

- Atomic radiation;
- Barometric pressure;

- Carbon dioxide concentration;
- Carbon monoxide concentration;
- Extremely Low Frequency (ELF) radiation;
- Nitrogen dioxide concentration;
- Ozone concentration;
- Particulate concentration;
- Percent relative humidity;
- Sound level;
- Sulfur dioxide concentration;
- Temperature; and,
- Ultraviolet radiation.

Each of the ACCESS parameters which appear in this report are discussed in detail below. Statistical summaries of the data collected are provided as an integral part of the program, and allows for data to be displayed graphically where applicable. Since it is difficult to display roughly 1500 data points at a time, an averaging technique is used to compress several minutes into one data point. This is why the first data point on a graph may not necessarily have the same value as that displayed after the first averaging period.

Please note that there are other pollutants which aren't measured by the EMS. Chlordane, VOC's, formaldehyde, lead and bacteria are among this group. If you are experiencing health problems which you suspect may be attributed to these pollutants, further sampling may be warranted.

A number of the indoor air quality standards and recommendations have been formulated by the American Society of Heating, Refrigerating and Air-Conditioning Engineers (ASHRAE). The upper and lower limits used in this report are in many cases derived from the most recent ASHRAE standard, ASHRAE 62-1989. Limits associated with outdoor air quality come from the Environmental Protection Agency's National Ambient Air Quality Standard (EPA-NAAQS) and the World Health Organization (WHO).


## STATISTICS

### Barometric Pressure

There are no standards for barometric pressure. Generally, a trend from high to low pressure signifies that unsettled weather is approaching. A trend in the opposite direction indicates fair weather is approaching.

Average value: 30.84 in.-Hg  
 Minimum value: 30.83 in.-Hg occurred on 3/6/2000 at 4:49:04 PM  
 Maximum value: 30.85 in.-Hg occurred on 3/6/2000 at 4:25:04 PM  
 Standard Deviation: 0.01 in.-Hg  
 Upper Limit: None  
 Lower Limit: None

## Barometric Pressure

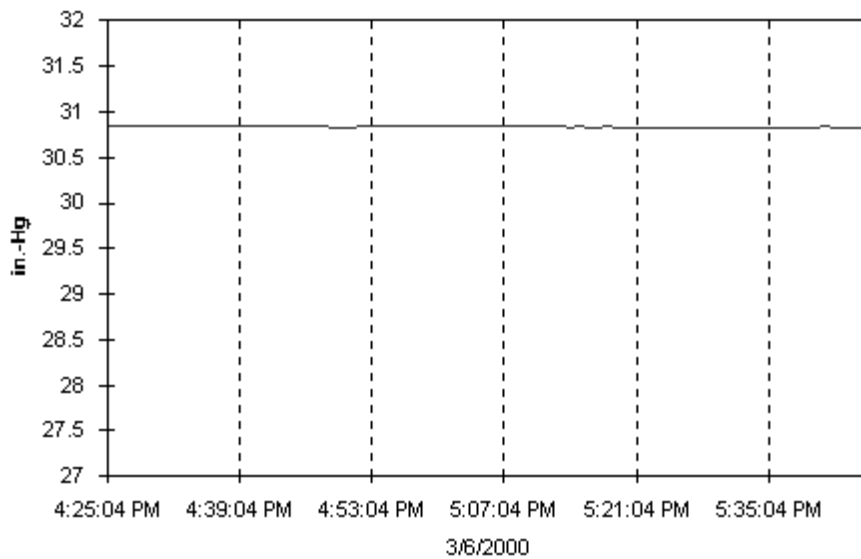

## Carbon Monoxide

Carbon monoxide (CO) is a toxic, odorless gas which is a fossil fuel combustion by-product. Primary residential sources of CO include gas stoves, unvented gas and kerosene space heaters, and wood stoves as well as from gas and oil furnaces and hot water heaters.

CO exposure is believed to contribute to, and in some cases worsen, heart disease. Particularly vulnerable are people with arteriosclerosis, and those who smoke cigarettes.

The National Ambient Air Quality Standard (EPA-NAAQS) places an upper limit of 9 ppm of CO for any eight hour period and a limit of 35 ppm for any one hour period.

Average value: .00 ppm

Minimum value: 0 ppm occurred on 3/6/2000 at 4:25:04 PM

Maximum value: 0 ppm occurred on 3/6/2000 at 4:25:04 PM

Standard Deviation: 0.00 ppm


Upper Limit: 9 ppm

Overlimit Occurrences: 0

Percent of total samples that were overlimit: 0. %

Lower Limit: None

## Carbon Monoxide

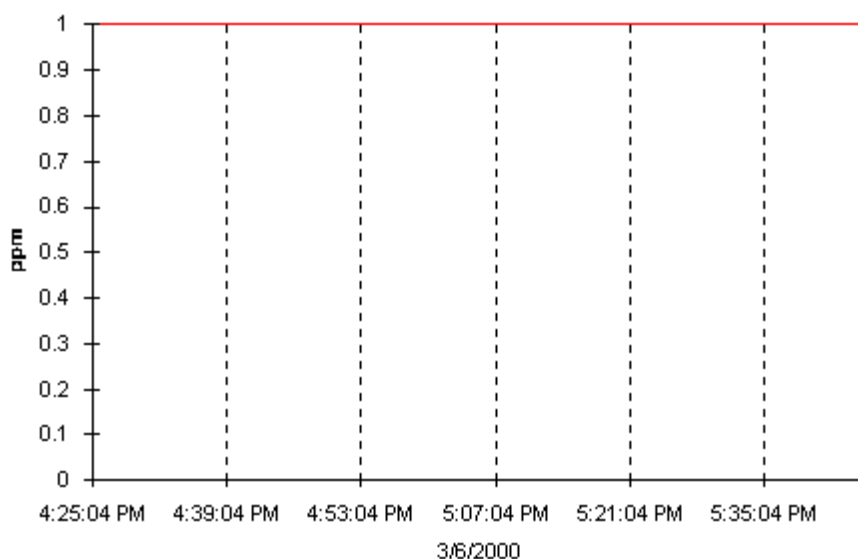

## Nitrogen Dioxide


Nitrogen dioxide (NO<sub>2</sub>) is a gas which is a combustion by-product. Cigarette smoke is a significant source of NO<sub>2</sub> in indoor air. There is no indoor air standard for NO<sub>2</sub> concentration. The NAAQS limits the annual mean value to 50 parts per billion (ppb) for outdoor air. Indoor levels can be considerably higher, exceeding 1,000 ppb during meal preparation which involve cooking. Average indoor concentrations may exceed 100 ppb over a period of days.

Urban outdoor concentration levels are usually between 10 and 50 ppb, according to the World Health Organization (WHO). The WHO recommends that the maximum one hour exposure level be under 210 ppb.

Since NO<sub>2</sub> combines readily with oxygen and other chemicals, isolating its health effects is difficult. The photochemical oxidants that it helps to create have varying degrees of toxicity. NO<sub>2</sub> contributes to respiratory illnesses, especially in people who are already vulnerable due to bronchitis, asthma or other lung disease.

Average value: 36.45 ppb  
Minimum value: 0 ppb occurred on 3/6/2000 at 5:16:04 PM  
Maximum value: 103 ppb occurred on 3/6/2000 at 4:25:04 PM  
Standard Deviation: 35.56 ppb  
Upper Limit: 80 ppb  
Overlimit Occurrences: 14  
Percent of total samples that were overlimit: 17.1 %  
Lower Limit: None

## Nitrogen Dioxide

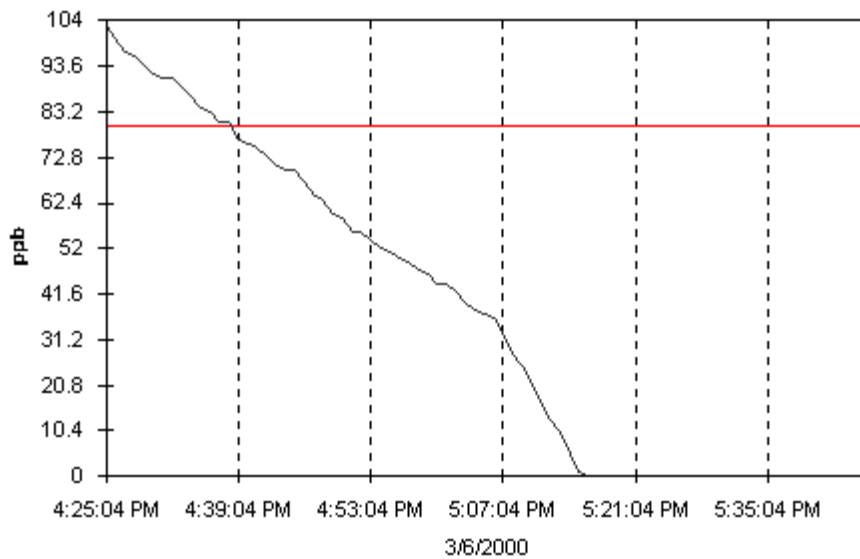

## Ozone

Ground-level ozone (O<sub>3</sub>) is a pollutant which can cause respiratory problems. The Food and Drug Administration (FDA) suggests that the indoor ozone concentration should be less than 50 parts per billion (ppb). The NAAQS designates a maximum concentration of 120 ppb for any one hour period.

As ozone levels rise, a continuum of less to more severe symptoms are reported, starting with dry throats, wheezing and eye irritation. Breathing may then become more labored, especially while exercising. At levels above 20 ppb, the potential for asthmatic attacks increases, athletic performance decreases significantly, and the impact of infectious illnesses is worsened. All of these effects are magnified for those who smoke cigarettes.

Average value: 1.10 ppb

Minimum value: 0 ppb occurred on 3/6/2000 at 4:37:04 PM

Maximum value: 2 ppb occurred on 3/6/2000 at 4:25:04 PM

Standard Deviation: 0.71 ppb


Upper Limit: 120 ppb

Overlimit Occurrences: 0

Percent of total samples that were overlimit: 0. %

Lower Limit: None

## Ozone

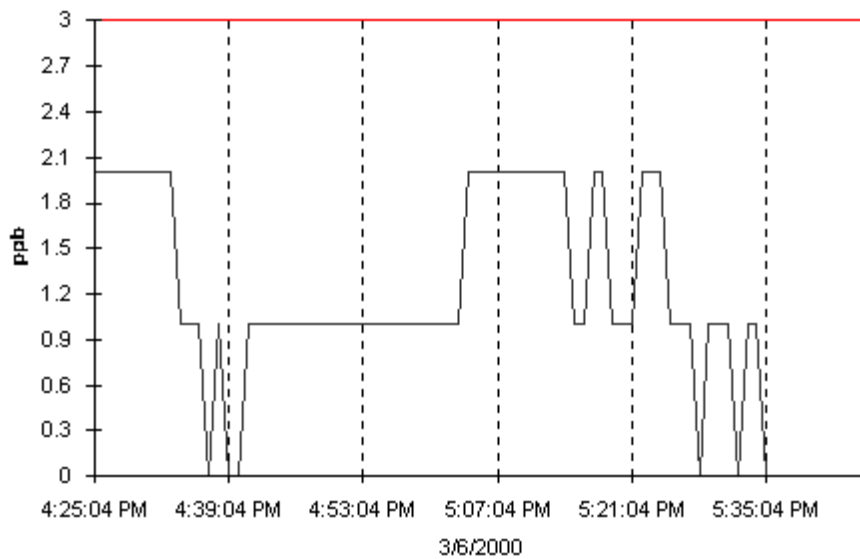

## Relative Humidity

ASHRAE 62-1989 suggests maintaining an indoor relative humidity between 30 and 60%. A relative humidity higher than 60% encourages the growth of mold and other biogenic pollutants while a humidity below 30% may cause irritation to mucous membranes due to a lack of moisture in the air.

Average value: 11.49 %

Minimum value: 6 % occurred on 3/6/2000 at 4:25:04 PM

Maximum value: 14 % occurred on 3/6/2000 at 5:26:04 PM

Standard Deviation: 2.04 %

Upper Limit: 60 %

Overlimit Occurrences: 0


Percent of total samples that were overlimit: 0. %

Lower Limit: 30 %

Underlimit Occurrences: 82

Percent of total samples that were underlimit: 100. %

### Relative Humidity

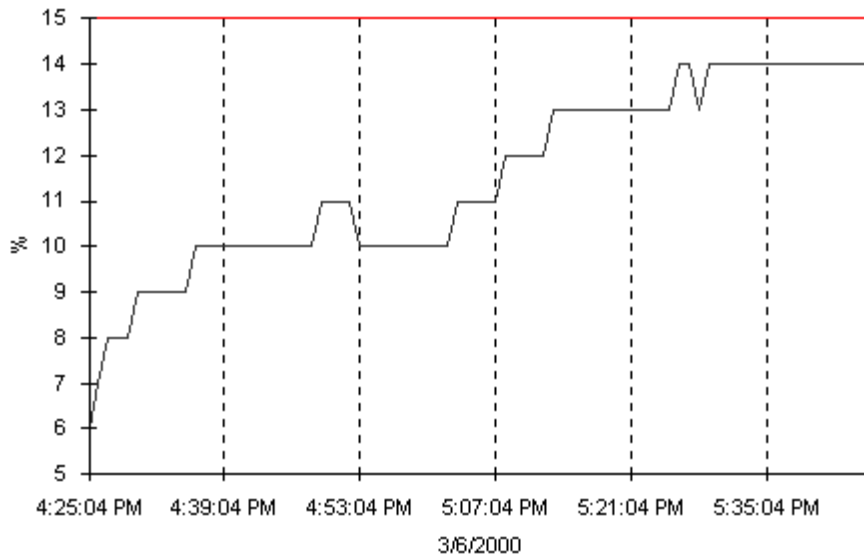

### Sulfur Dioxide

A combustion by-product of wood-burning stoves and hydrocarbon fuels, sulfur dioxide (SO<sub>2</sub>) is a toxic gas. The NAAQS requires SO<sub>2</sub> concentration to be below 140 parts per billion (ppb) in any given 24 hour period. In some parts of Europe, twenty four hour background levels are between 85 and 170 ppb, according to the WHO.

Elevated levels of SO<sub>2</sub> contribute to a variety of respiratory ailments. Chronic, long-term low-level exposure to SO<sub>2</sub> is a contributing factor leading to bronchitis, lung cancer and labored breathing. Frequency and severity of respiratory disease also increases. The ability of the lungs to filter out particles, bacteria and harmful microorganisms is reduced. Lung damage can be irreversible.

Average value: .00 ppb

Minimum value: 0 ppb occurred on 3/6/2000 at 4:25:04 PM

Maximum value: 0 ppb occurred on 3/6/2000 at 4:25:04 PM

Standard Deviation: 0.00 ppb


Upper Limit: 140 ppb

Overlimit Occurrences: 0

Percent of total samples that were overlimit: 0. %

Lower Limit: None

### Sulfur Dioxide

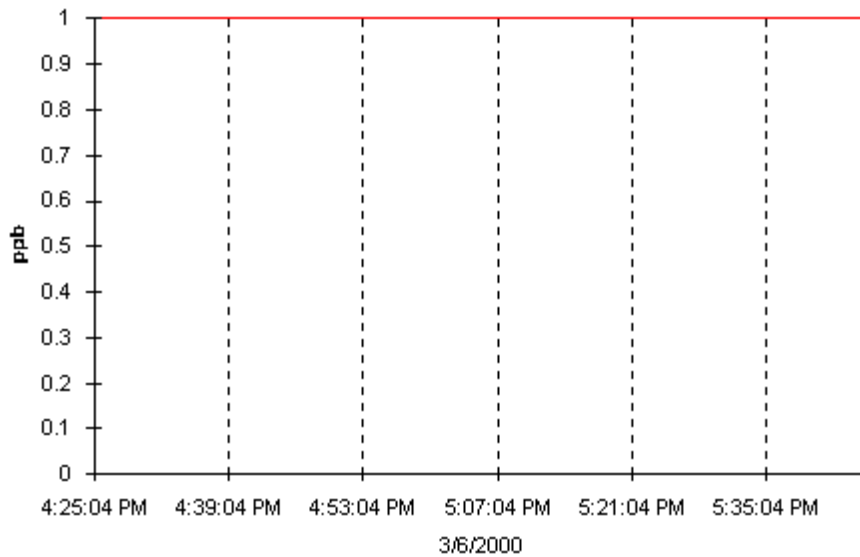


### Temperature

Comfortable indoor temperature is a subjective factor and there are no standards for indoor air temperature. It should be noted however, that lower temperatures will tend to inhibit the release of both volatile organic compounds, (found in construction materials, paints, and furnishings), and formaldehyde. Values between 65°F and 75°F are considered 'comfortable' by a majority of people.

Average value: 57.83 Deg. F  
Minimum value: 53 Deg. F occurred on 3/6/2000 at 5:45:04 PM  
Maximum value: 67.7 Deg. F occurred on 3/6/2000 at 4:25:04 PM  
Standard Deviation: 3.78 Deg. F  
Upper Limit: None  
Lower Limit: None


### Temperature

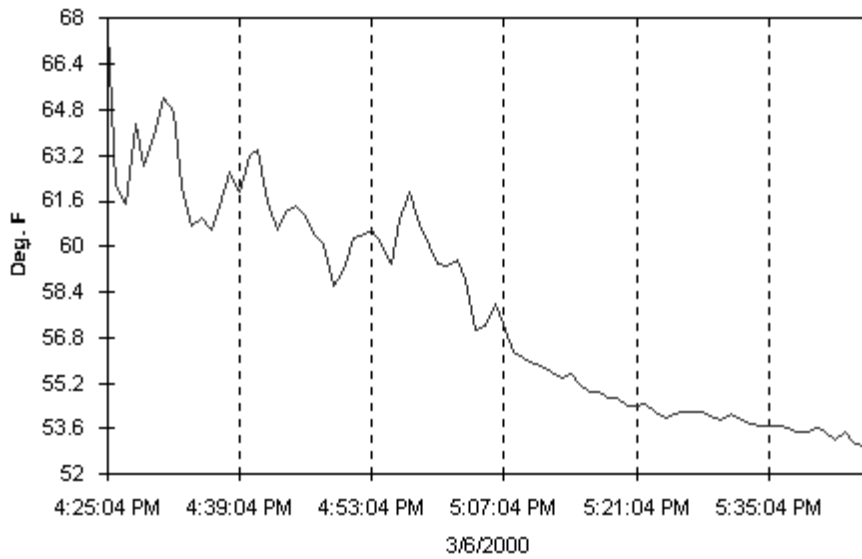

### Wind Direction

Average value: 260.15 Deg.  
Minimum value: 3 Deg. occurred on 3/6/2000 at 4:32:04 PM  
Maximum value: 359 Deg. occurred on 3/6/2000 at 5:34:04 PM  
Standard Deviation: 122.06 Deg.  
Upper Limit: None  
Lower Limit: None


### Wind Direction

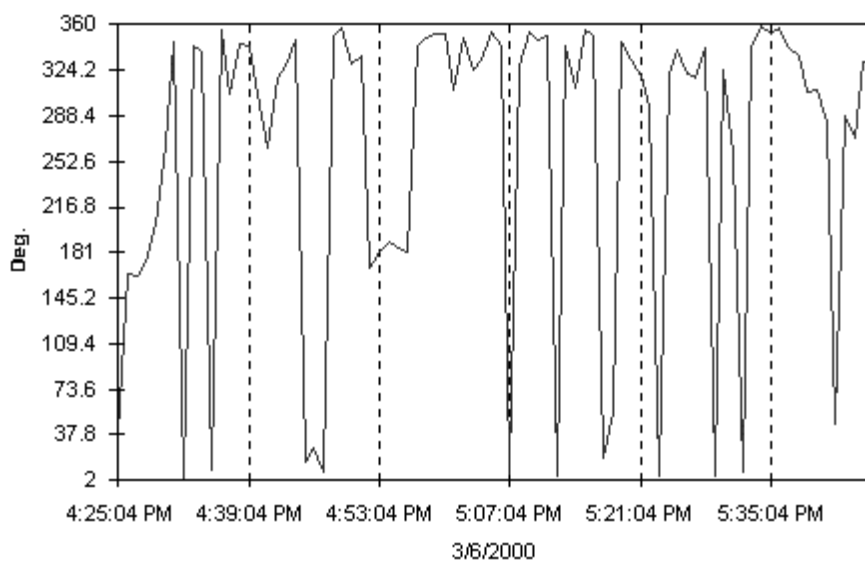

### Wind Speed

Average value: 2.89 mph  
Minimum value: 0 mph occurred on 3/6/2000 at 4:31:04 PM  
Maximum value: 6 mph occurred on 3/6/2000 at 4:49:04 PM  
Standard Deviation: 1.39 mph  
Upper Limit: None  
Lower Limit: None

### Wind Speed

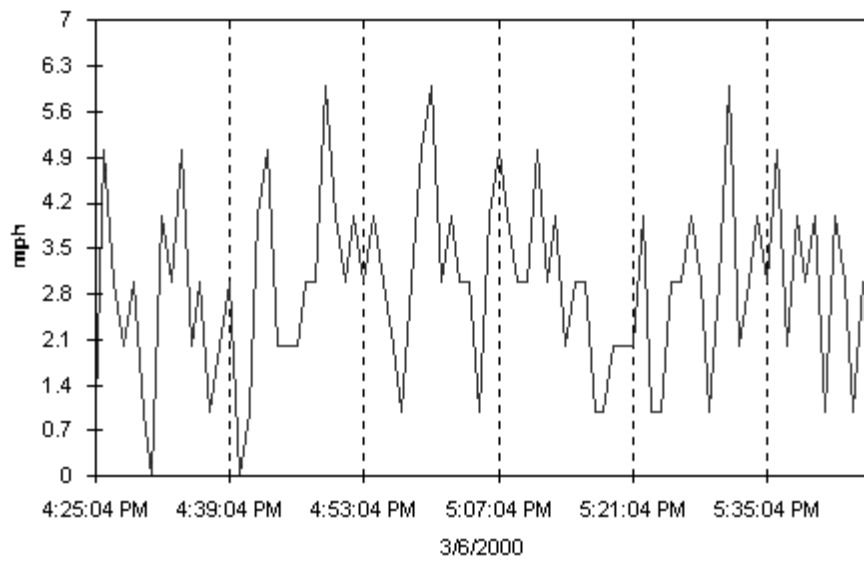

### Supply Voltage

Average value: 12.01 V  
Minimum value: 11.81 V occurred on 3/6/2000 at 5:41:04 PM  
Maximum value: 12.16 V occurred on 3/6/2000 at 4:25:04 PM  
Standard Deviation: 0.08 V  
Upper Limit: None  
Lower Limit: None

### Supply Voltage

